


SALES DRAWING ONLY
NOT TO BE USED FOR MANUFACTURE

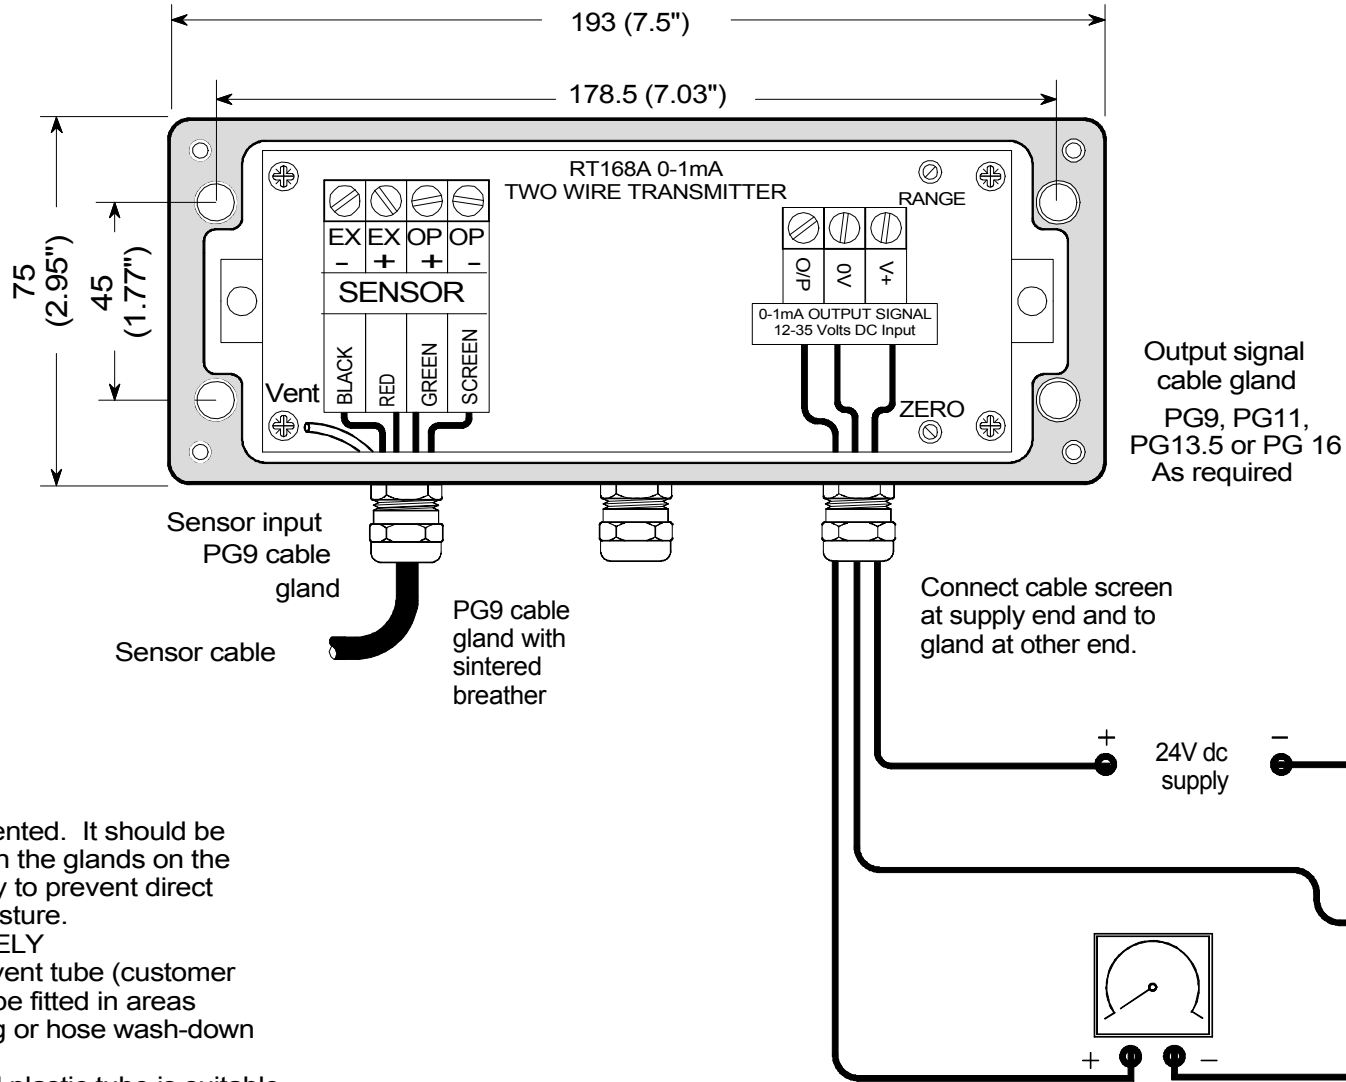

IMPORTANT
The case is vented. It should be positioned with the glands on the underside only to prevent direct ingress of moisture.
ALTERNATIVELY
An extended vent tube (customer supply) must be fitted in areas where flooding or hose wash-down are likely.
6mm (1/4") od plastic tube is suitable and should run to a dry area.
(The sintered plug may be removed in this case)

PSm Instrumentation Ltd

Haywards Heath, West Sussex RH16 1TW
ph: 44 (0) 1444 410040 f: 44 (0) 1444 410121
<http://www.psm-sensors.co.uk>

SCALE
NTS

UNLESS OTHERWISE STATED DIMENSIONS ARE IN
MILLIMETRES / INCHES

TITLE
260/360 SERIES 0 to 1 mA
Connection diagram

DRAWING NO
S001098-360-DD

A4

SHT 1
OF 1

ISSUE	DATE	DCR	DRAWN	CHECKED
A	15-01-99		JEK	JEK
B	18-09-00		JEK	JEK
C	17-07-02		JEK	JEK